

FIG. 1

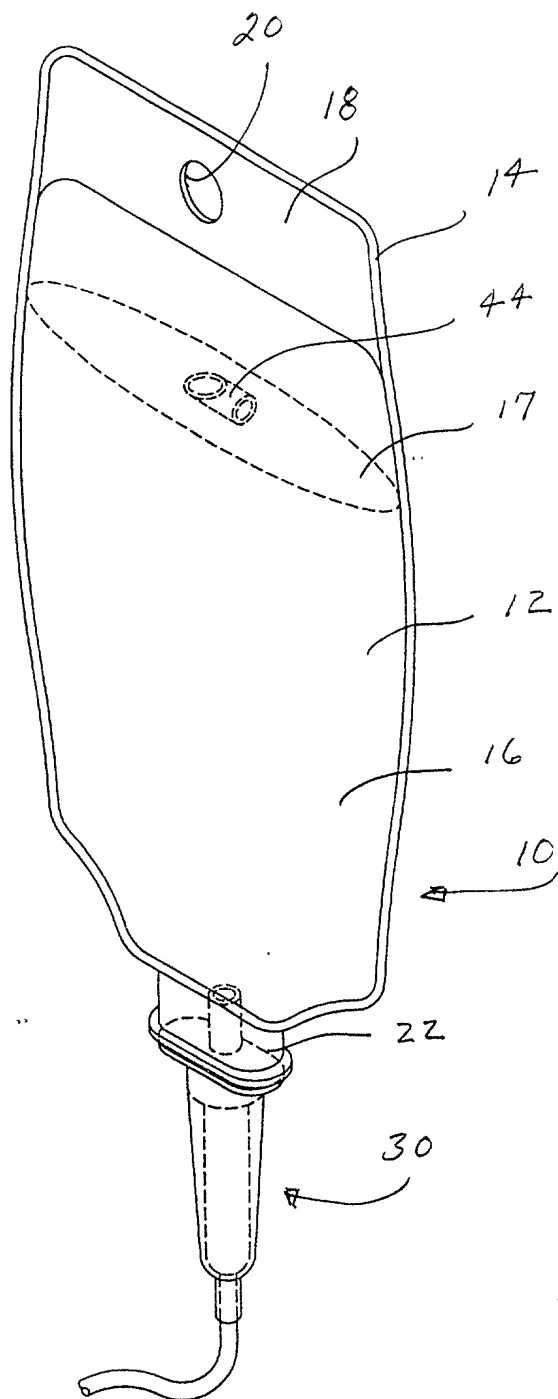


FIG. 1A

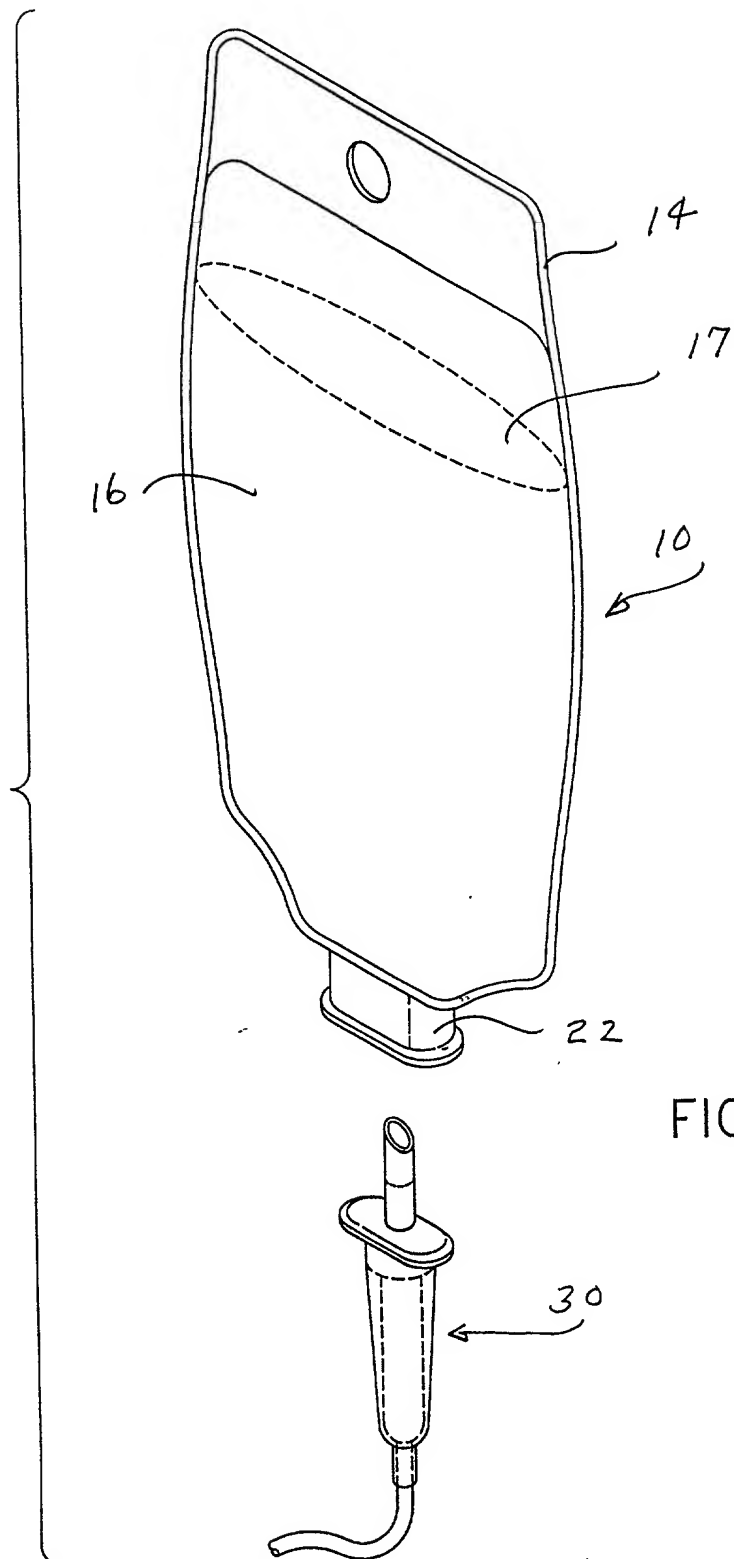


FIG. 2

FIG. 3 is a perspective view of the device 10 in a closed position, showing the housing 12, the plunger 30, and the needle 32. The device 10 is shown in a closed position, with the plunger 30 and the needle 32 retracted into the housing 12. The housing 12 is shown with a top cap 14 and a bottom cap 16. The plunger 30 is shown with a top cap 34 and a bottom cap 36. The needle 32 is shown with a top cap 38 and a bottom cap 40.


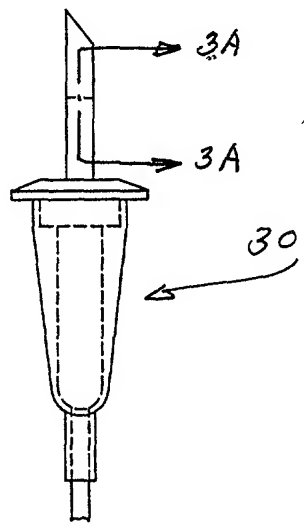
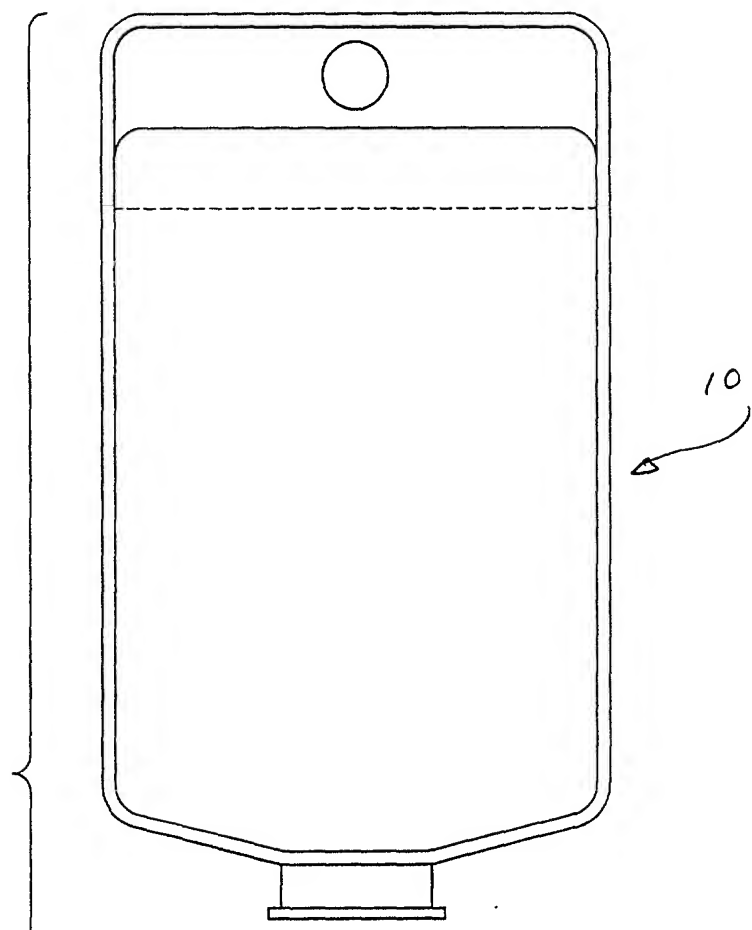


FIG. 3

FIG. 3A

FIG. 4

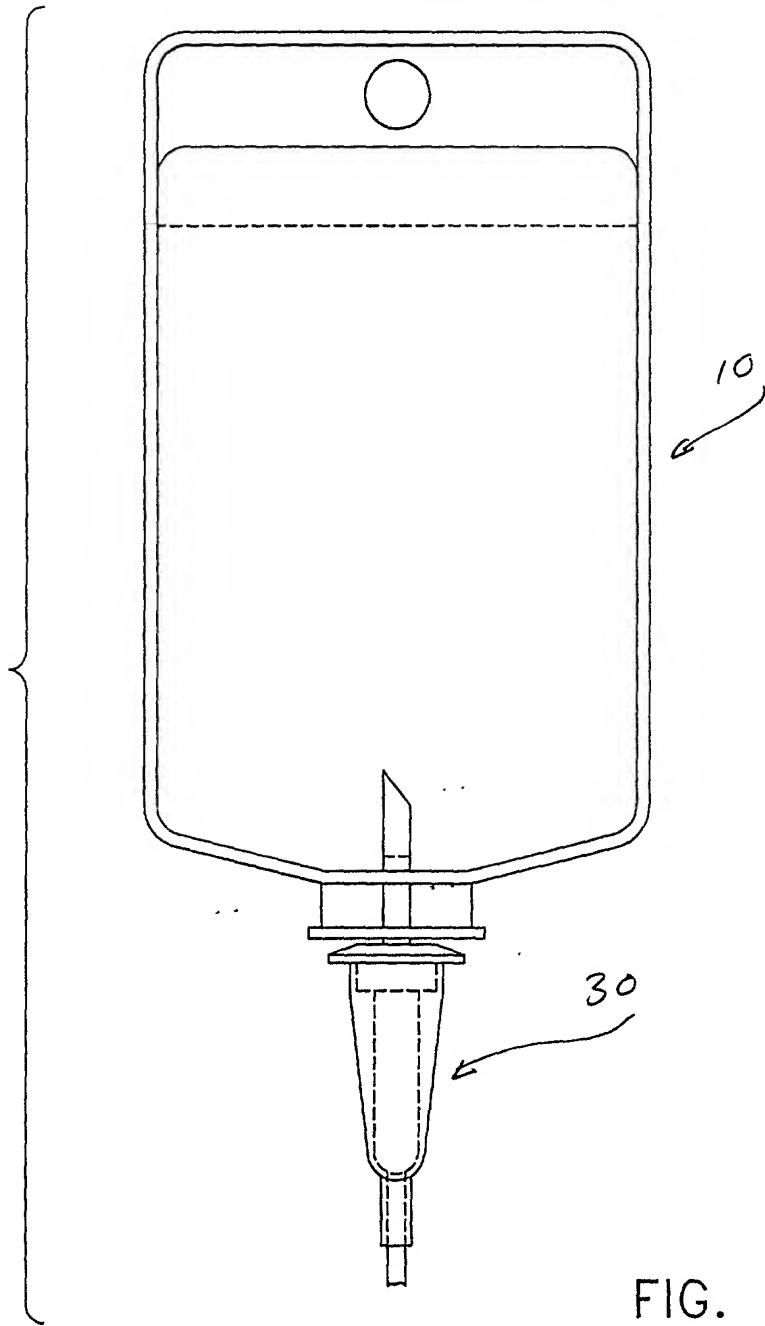
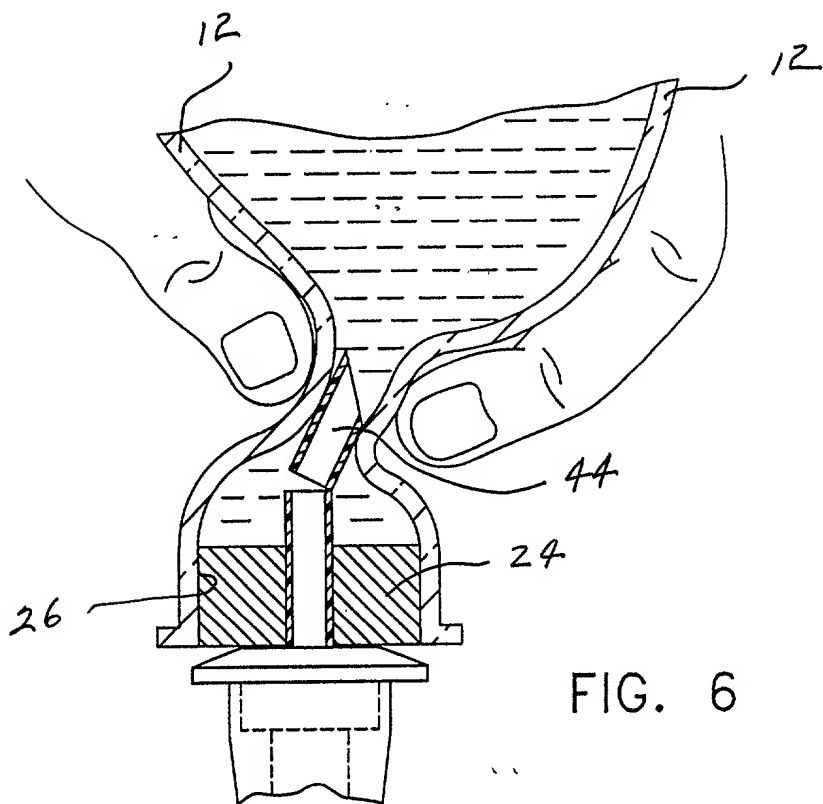
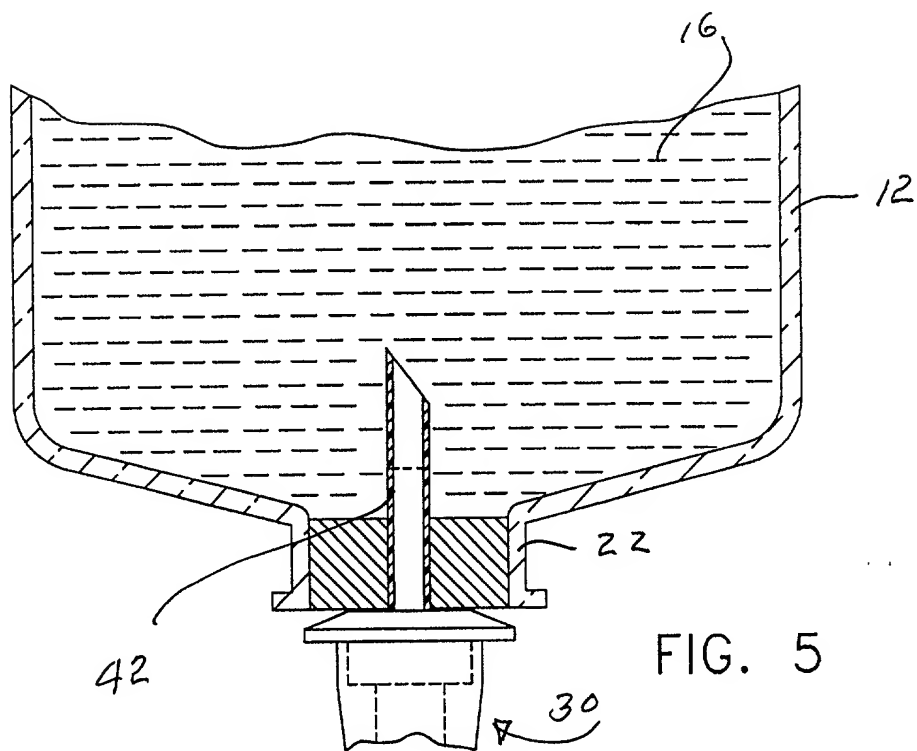


FIG. 4



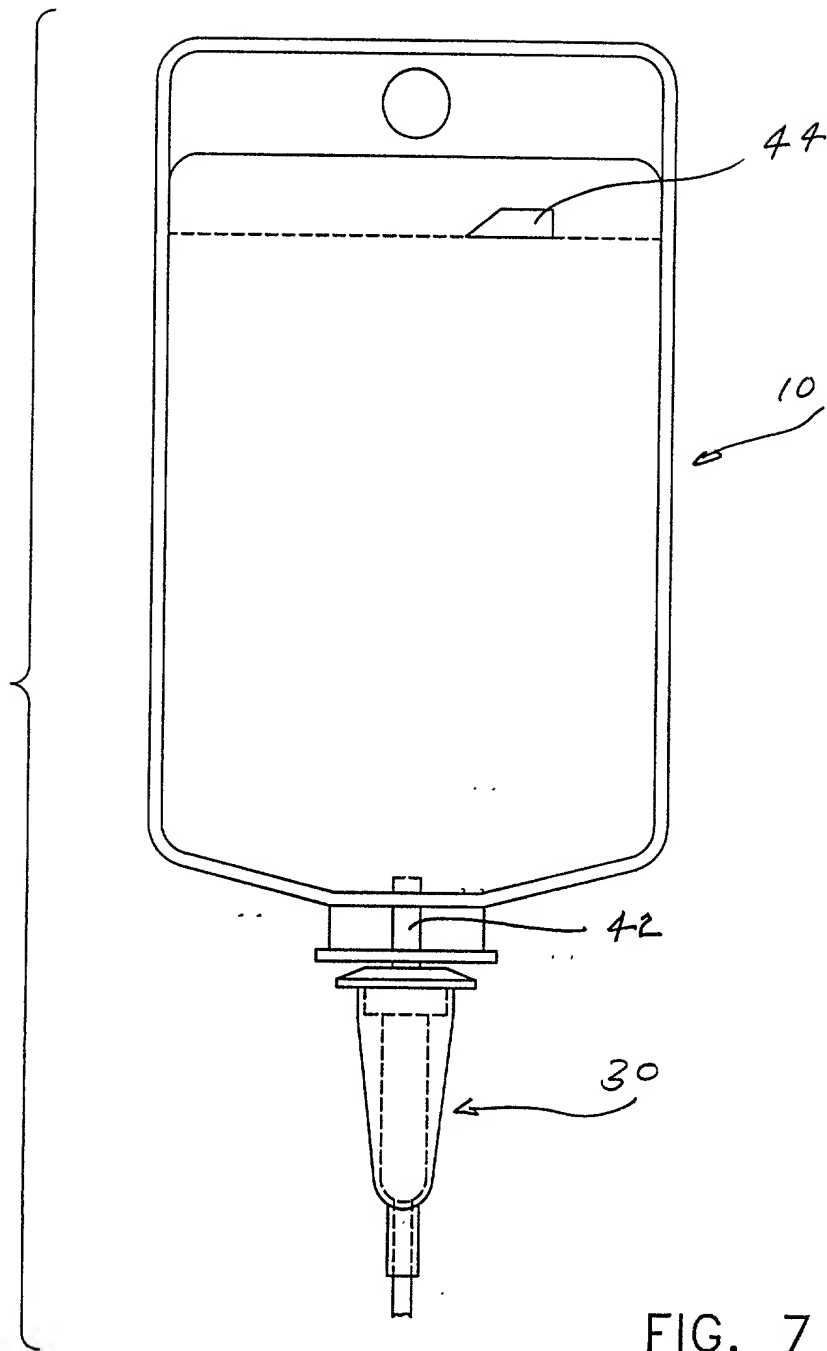


FIG. 7

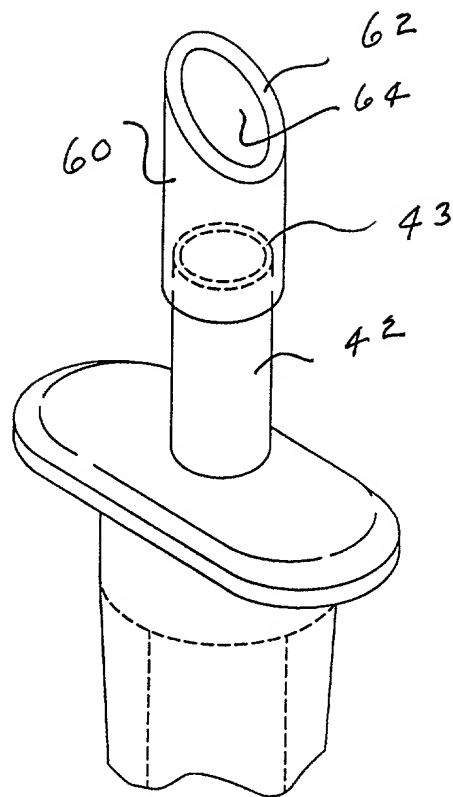


FIG. 8

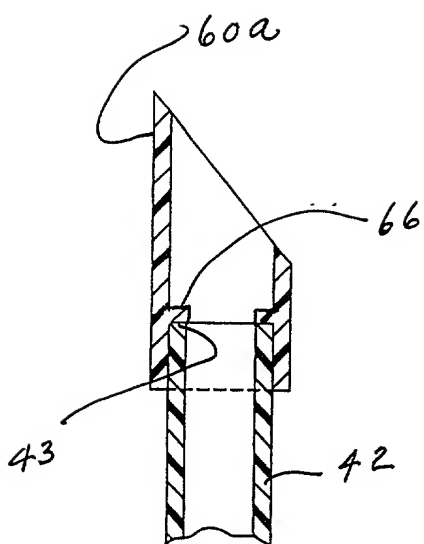


FIG. 8A

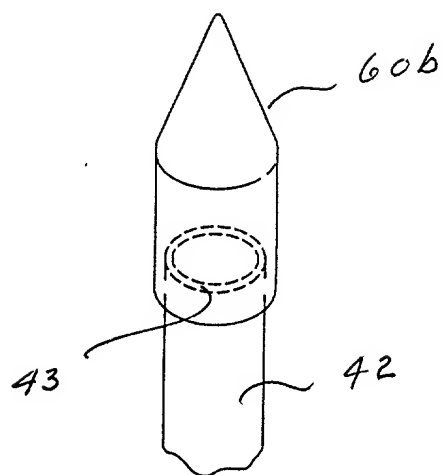


FIG. 8B

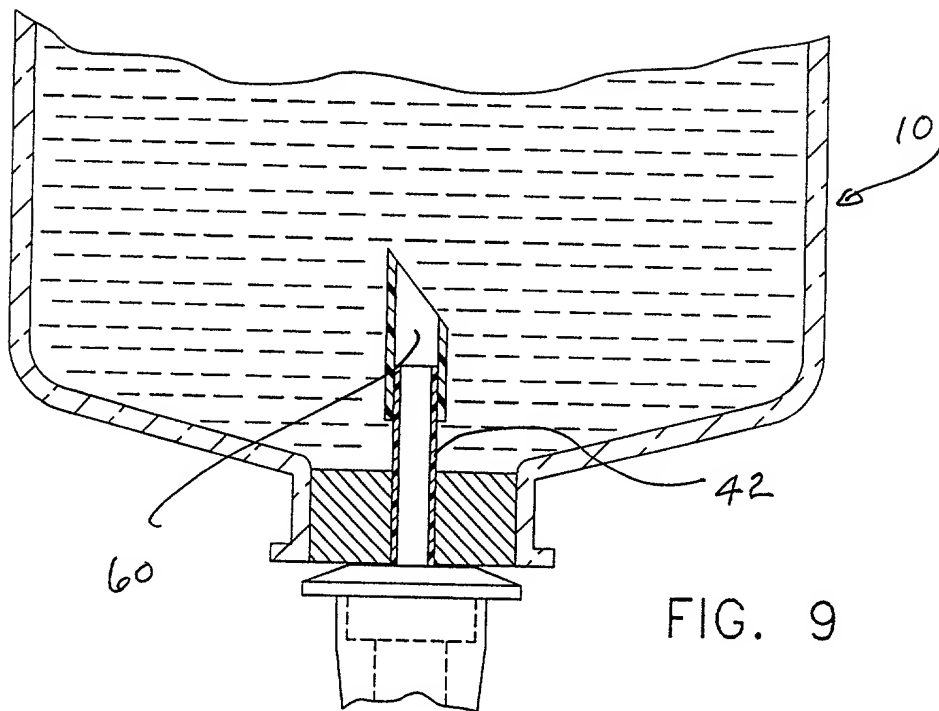


FIG. 9

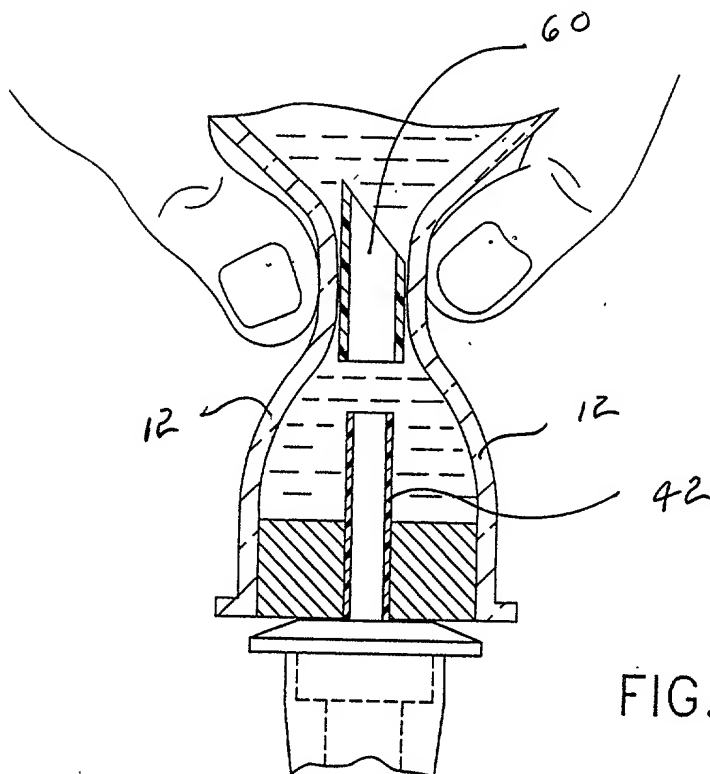


FIG. 10

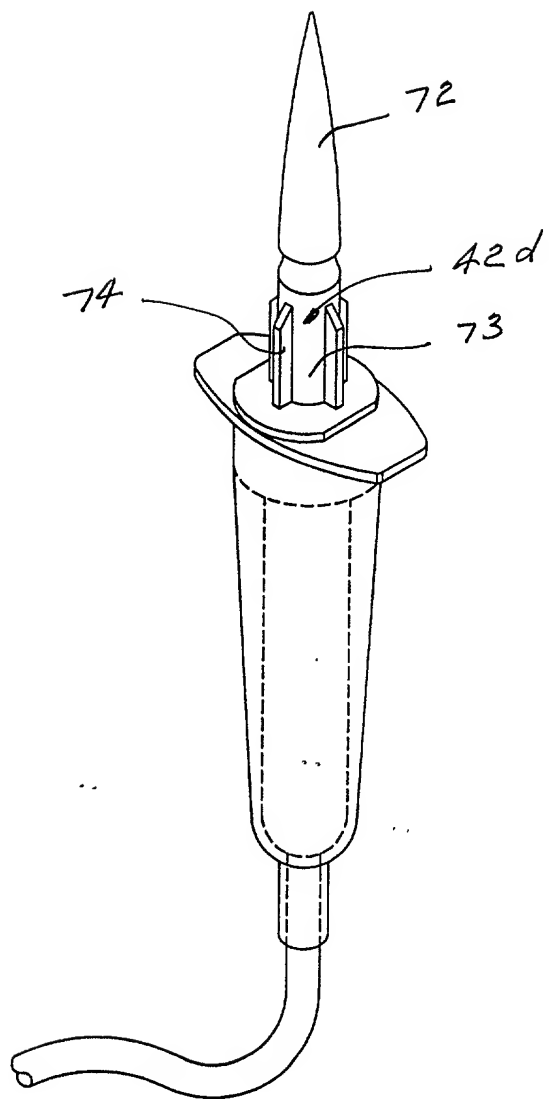


FIG. 11

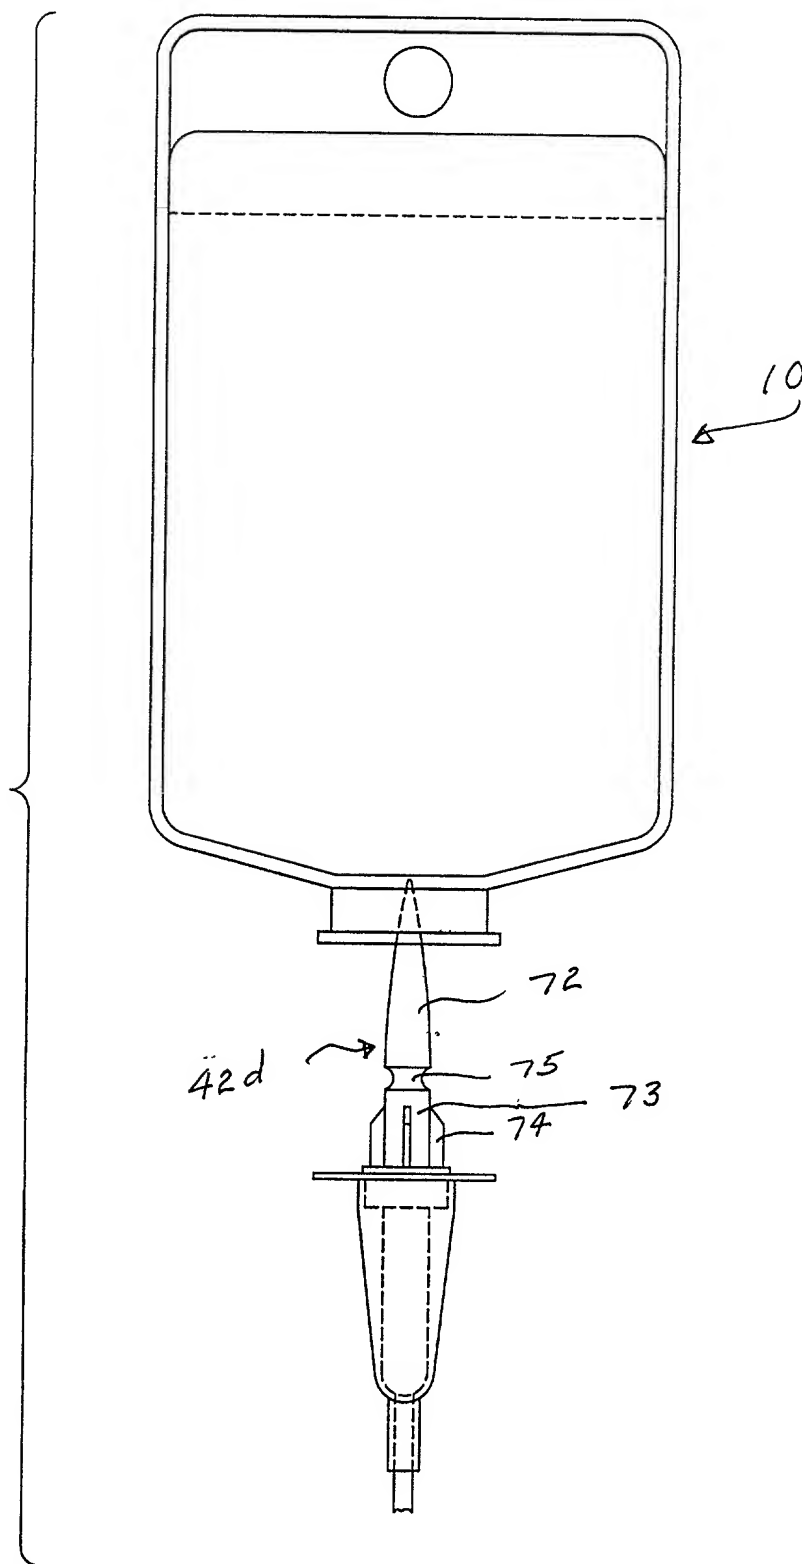


FIG. 12 "

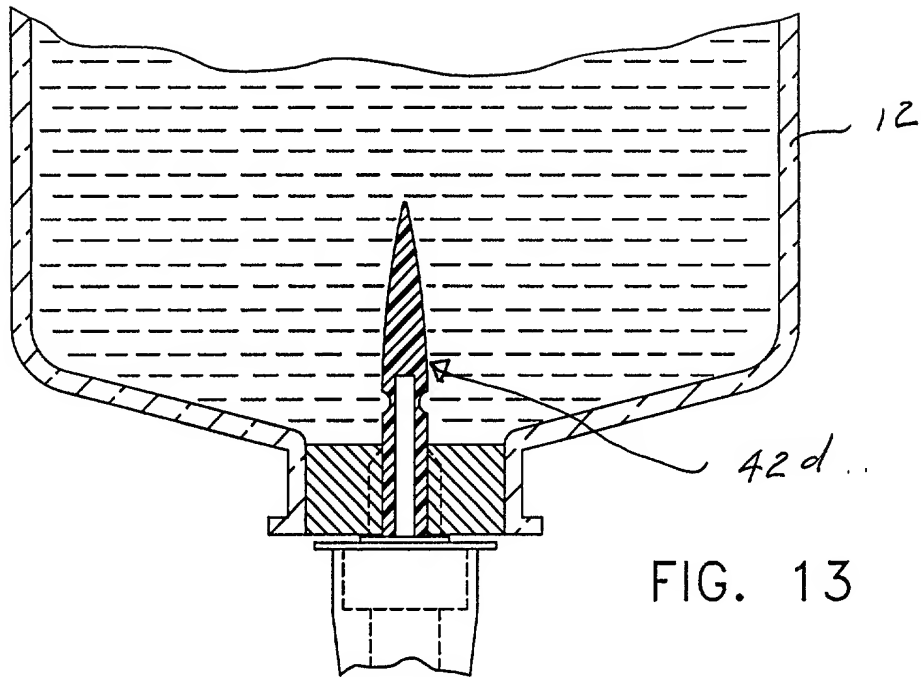


FIG. 13

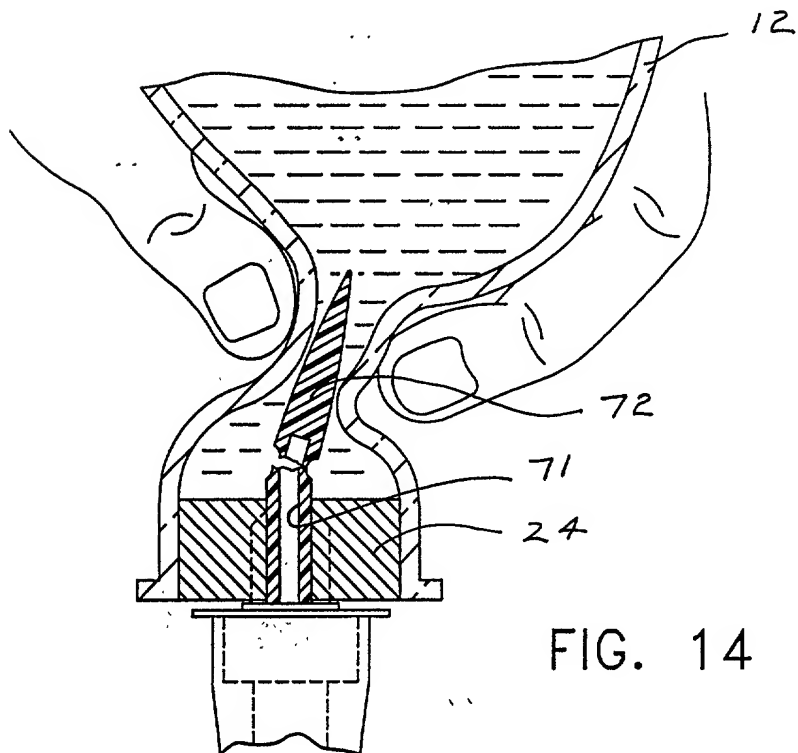


FIG. 14

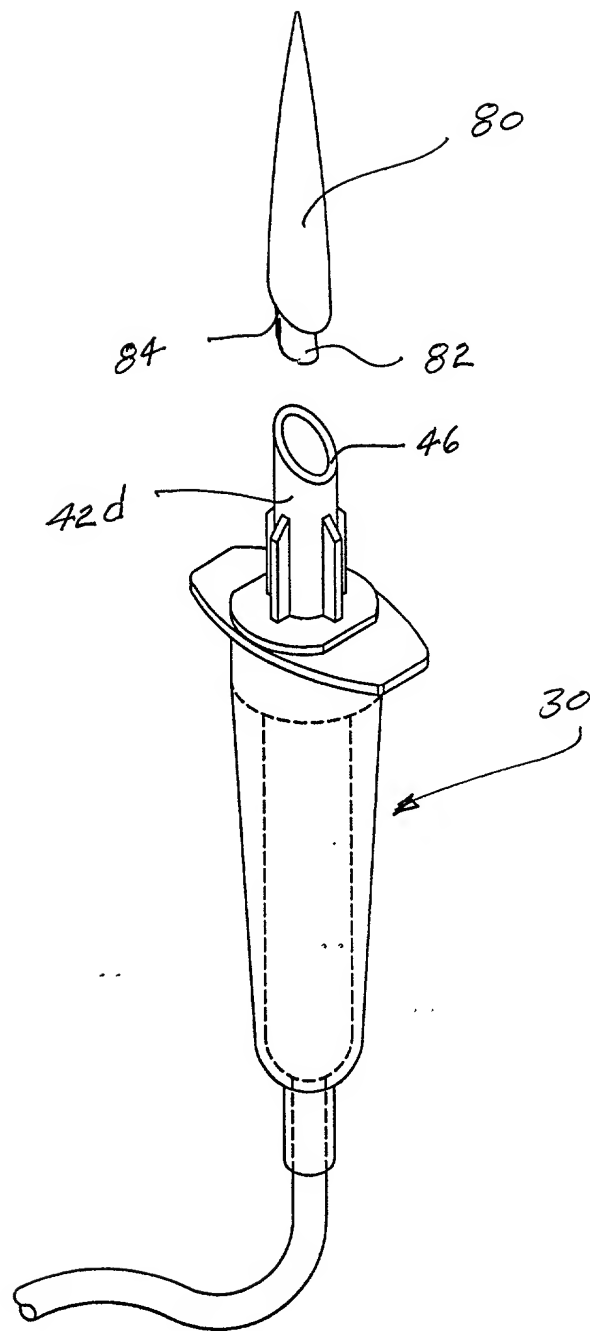


FIG. 15




FIG. 15A

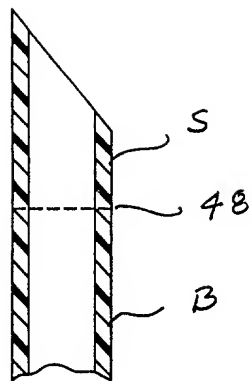


FIG. 16A

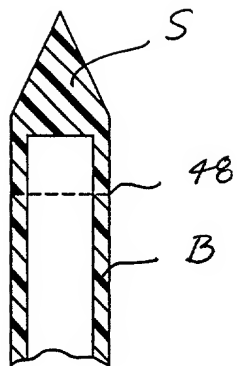


FIG. 16B

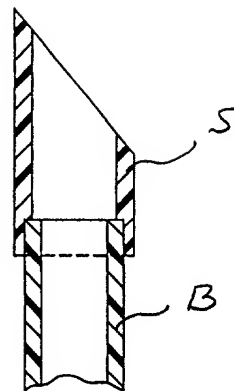


FIG. 16C

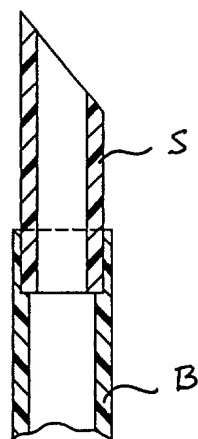


FIG. 16D

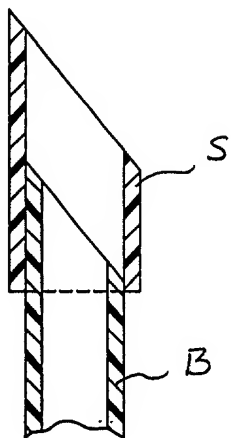


FIG. 16E

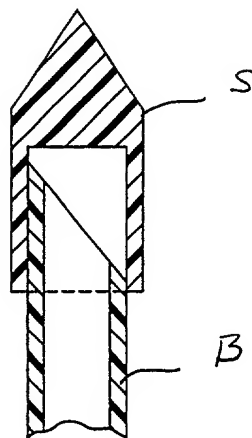


FIG. 16F

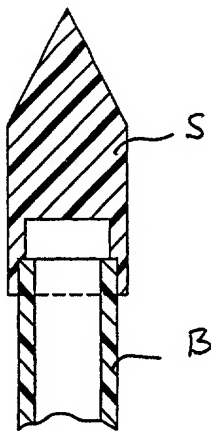


FIG. 16G

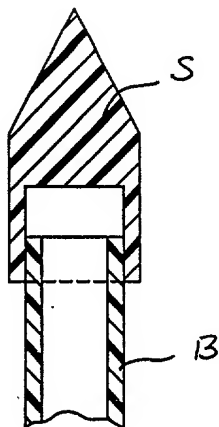


FIG. 16H

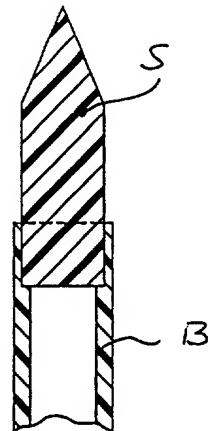


FIG. 16I